

TYRUKO (natalizumab)

TREATMENT CONTINUATION FORM

This medicine is subject to additional monitoring. This will allow quick identification of new safety information.

This form should be read carefully before continuing NATALIZUMAB treatment for more than 2 years. Although you have been receiving NATALIZUMAB for 2 years, it is important that you are reminded that the risk of PML increases beyond this time. Please follow the advice in this form to ensure that you are fully informed of, and understand the risk of PML (progressive multifocal leukoencephalopathy), IRIS (immune reconstitution inflammatory syndrome) and other important adverse effects of NATALIZUMAB.

Before continuing treatment with NATALIZUMAB you should:

- **Read the Patient Leaflet which is included in each box of TYRUKO**
- **Read the Alert Card given to you by your doctor**
- **Discuss with your doctor the benefits and the risks associated with this treatment**

The Patient Leaflet and the Alert Card contain important safety information about PML, a rare brain infection that has occurred in patients who have been given natalizumab, and which may lead to severe disability or death. PML is associated with an uncontrolled increase of the JC virus in the brain, although the reason for this increase in some patients treated with natalizumab is unknown. JC virus is a common virus which infects many people but does not normally cause noticeable illness.

The risk of PML with NATALIZUMAB is higher:

- If you have antibodies to the JC virus in your blood
- The longer that you are on treatment with NATALIZUMAB, especially if you have been on treatment for more than 2 years
- If you have taken an immunosuppressant (a medicine that reduces the activity of your body's immune system) at any time before starting NATALIZUMAB treatment

Your doctor should discuss the potential risk of developing PML with you before you continue treatment with NATALIZUMAB.

Your doctor may test your blood to check if you have antibodies to the JC virus before you continue treatment with NATALIZUMAB. Your doctor may repeat the test while you are on NATALIZUMAB treatment to check if anything has changed. The risk of PML is higher if you have all the risk factors described above, or if you have not taken an immunosuppressant medication prior to starting NATALIZUMAB and have higher levels of antibodies to the JC virus and you have been on NATALIZUMAB for more than 2 years. Your doctor will monitor you more closely if you are at higher risk for PML.

You should discuss with your doctor if NATALIZUMAB is the most suitable treatment for you before you continue NATALIZUMAB for more than 2 years.

In patients with PML, a reaction known as IRIS (immune reconstitution inflammatory syndrome) is likely to occur after treatment for PML, as natalizumab is removed from your body. IRIS may lead to your condition getting worse, including worsening of brain function.

The Patient Leaflet should be read each time that you take NATALIZUMAB because it may have new information that is important to your treatment.

You should keep the Alert Card with you to remind you of the important safety information, in particular any symptoms you may develop which could possibly indicate PML. If appropriate, you should show the Alert Card to your partner or caregiver.

If you do not have the Patient Leaflet or the Alert Card, then please ask your doctor to provide them to you before you receive your NATALIZUMAB treatment.

Patient's Name (print)

Patient's Signature


Date

Doctor's Name (print)

Doctor's Signature

Date

PML risk estimation:

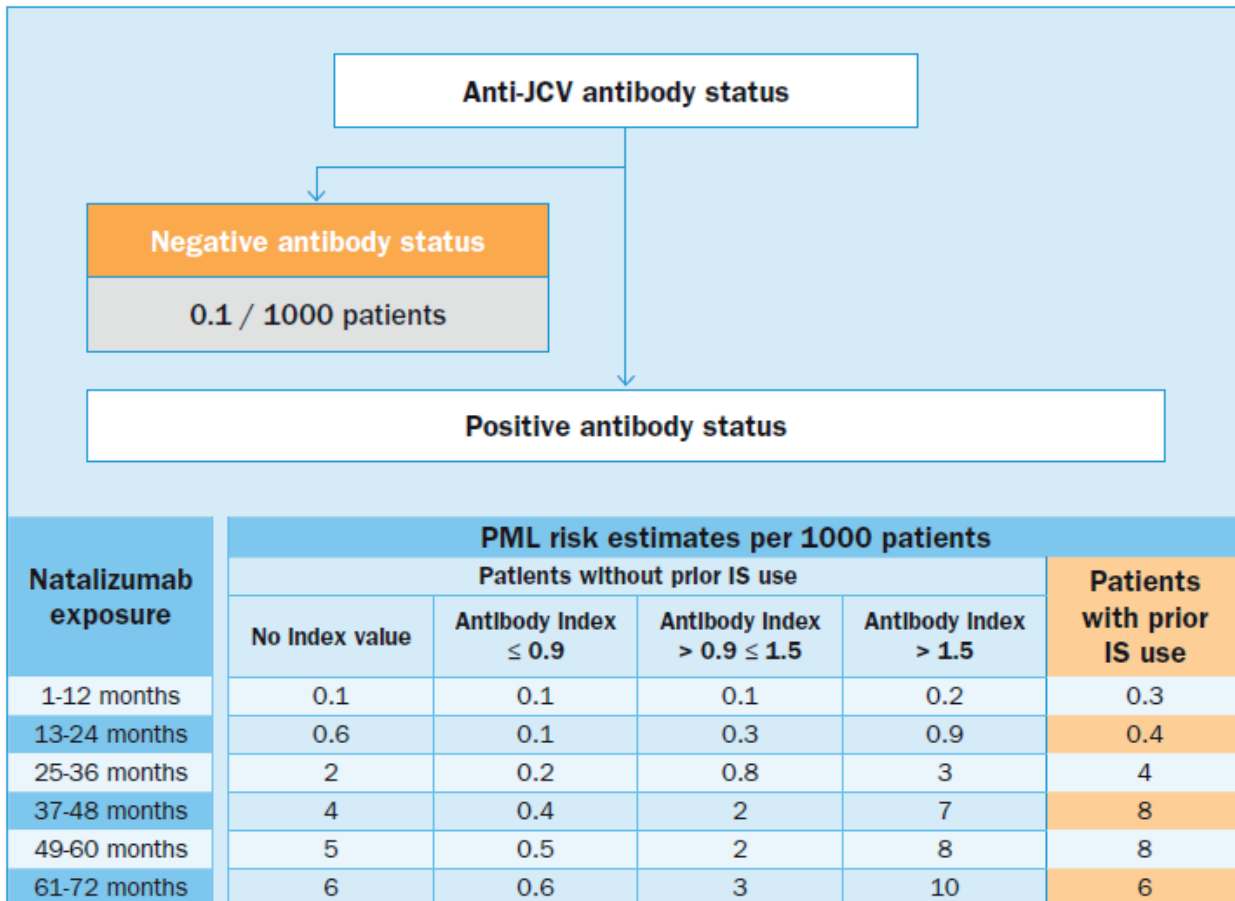

IS: Immunosuppressant

Anti-JCV antibody index values may depend on the assay used. The PML Risk Estimates provided above are based on anti-JCV antibody index data obtained from use of the STRATIFY JCV DxSelect assay.

An additional anti-JCV antibody assay, ImmunoWELL™ JCV IgG test, has been developed. The comparison between STRATIFY JCV® DxSelect® *, and ImmunoWELL JCV IgG tests indicates a potential offset of up to 0.1 in index values (e.g. lower range: 0.8, higher range: > 1.4 in the table above) when using the ImmunoWELL™ JCV IgG test.

*STRATIFY JCV® is a trademark of Biogen MA Inc. DxSelect® is a trademark of DIASORIN S.p.A.

Patients who are anti-JCV antibody negative

Based on the available data, if you do not have antibodies to JCV your chance of getting PML is 0.1/1000 (or 1 in 10,000) patients.

Patients who are anti-JCV antibody positive

If you do have antibodies to JCV, your risk of developing PML will vary depending on the duration of treatment with NATALIZUMAB, the level of anti-JCV antibodies in your blood and whether you have received prior treatment with an immunosuppressant medication. Your doctor will discuss the potential risk before you continue with treatment.

Reporting of side effects:

This medicine is subject to additional monitoring. This will allow quick identification of new safety information. You can help by reporting any side effects you may get. Please report suspected adverse drug reactions (ADRs) to the MHRA through the Yellow Card scheme. You can report via:

- the Yellow Card website www.yellowcard.mhra.gov.uk
- the free Yellow Card app available from the Apple App Store or Google Play Store
- some clinical IT systems (EMIS/SystemOne/Vision/MiDatabank) for healthcare professionals

Alternatively you can report a suspected side effect to the Yellow Card scheme by calling 0800 731 6789 for free, Monday to Friday between 9am and 5pm. You can leave a message outside of these hours.

When reporting please provide as much information as possible. By reporting side effects, you can help provide more information on the safety of this medicine.

Artwork Proof Box:		Technical Colours:	
Variation:	Initial Educational Material Registration + RFI 3	<input type="checkbox"/>	Legend:
Proof no:	001.3		
Date prepared:	05/12/2023		
Font size:	9.5pt		
Fonts:	Helvetica		
Dimensions:	210 x 297 mm		
Technical data:			
SKUs:	00000000		
SZ codes:	SZ0000000000		
Item codes:	00000000	Colours:	
Pharma codes:	00000000	<input checked="" type="checkbox"/>	Pantone 541
Novartis data if applicable:			
Version:	00000000		
Print Proof date:	00000000		
AQWA#:	00000000		
Production site:	00000000		
Technical num:	00000000		
Old Comp num:	00000000		



Signature Panel:	
<input type="text"/>	<input type="text"/>
<input type="text"/>	<input type="text"/>
<input type="text"/>	<input type="text"/>